


- ① Water Flow Meter*
- ② Softener*
- ③ Ro Unit
- ④ Storage tank
- ⑤ Deioniser cartridge*
- ⑥ Counter top tap and/or dispensing valve
- ⑦ Drain saddle valve

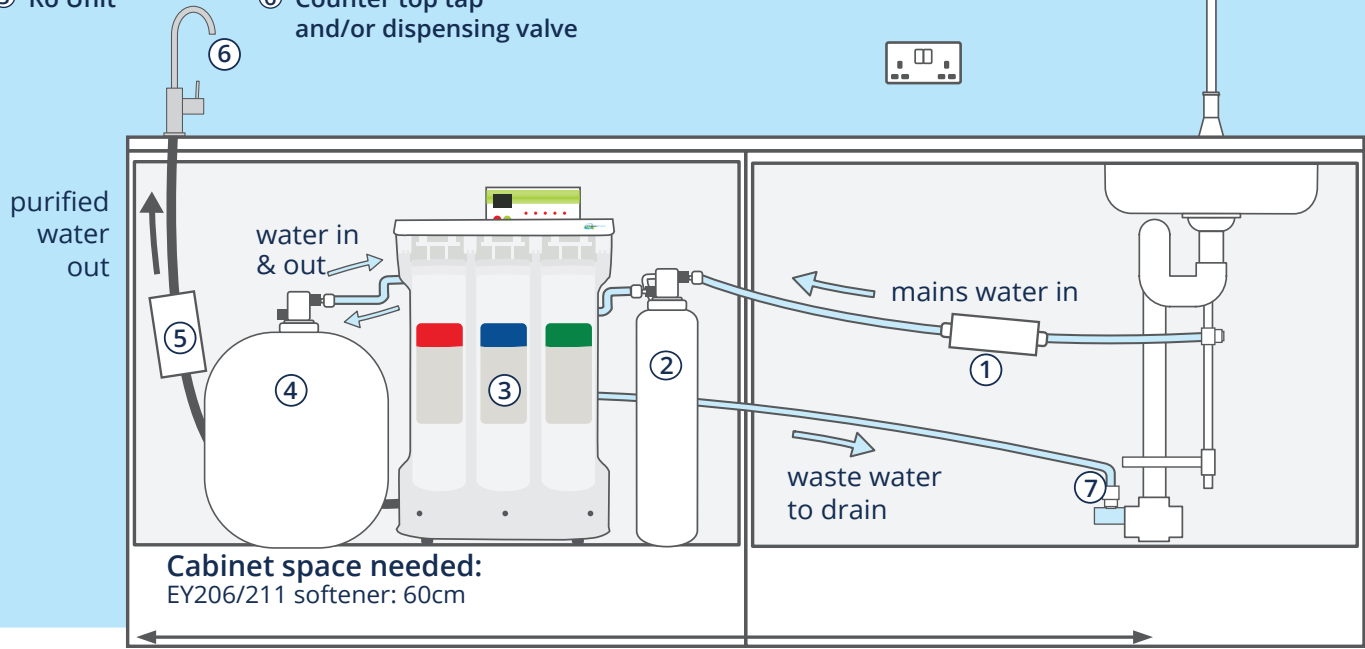

* Optional. See "What Reverse Osmosis (RO) components do I need for my autoclave model?" flow chart.
Recommended tank size depends on daily typical water usage: dental chair = 2L, autoclave = 5L.